


Set-Up Guide

Robotic FloShield Plus for the 8.5mm da Vinci Si HD

DISCONNECTING

Grip adapter, squeeze collar locking tabs, and apply **gentle pressure up** towards the scope.

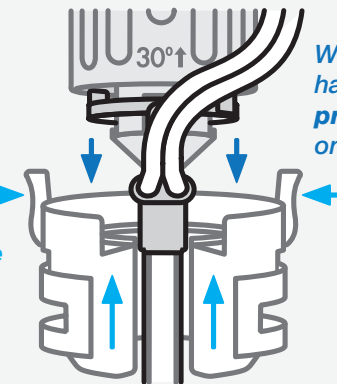

With opposite hand, put **gentle pressure down** on the scope.

Disengage the FloShield locking tabs, using a slight left-right twist to loosen.

Remove FloShield sheath from laparoscope.

